

Certificate of Analysis

Adria
Adria Science
Slovenia
info@adriascience.com
www.adriascience.com

Liquilabs s.r.o.
Inovační 122
252 41 Zlatníky-Hodkovice
Czechia
www.liquilabs.cz



[Verify Results Online](#)

Sample Identification

Sample Name Bacteriostatic Water 3 ml
Batch Number 2024214
Date Published 2026-07-27 16:19

Results for LIQ-0039

Stabilizers	Result	Unit	Uncertainty	Acceptable Range
Benzyl Alcohol Content Benzyl alcohol	1.03	%	[± 0.02]	0.9 - 1.1
Peptides	Result	Unit	Uncertainty	Acceptable Range
pH Determination pH determination	6.4		[± 0.1]	4.45 - 7
Microbiology	Result	Unit	Uncertainty	Acceptable Range
Bacterial Endotoxin Chromgenic USP<85>/ Eur. Ph. 2.6.14. Bacterial Endotoxin Chromgenic Test	0.008	EU/g	[± 0]	<= 0.25

Analysis Report




Sample Information


Injection Volume : 1
Data File : LIQ-0039_002.lcd
Method File : Benzylalcohol v2.0.lcm
Date Acquired : 23.07.2026 13:45:47

Chromatogram

uV

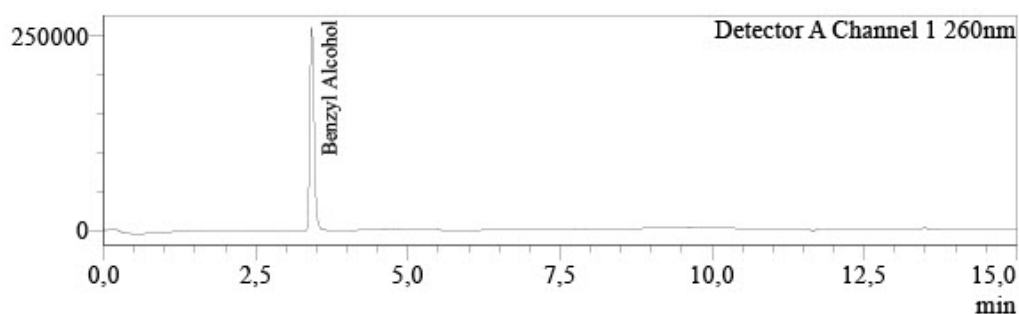

uV

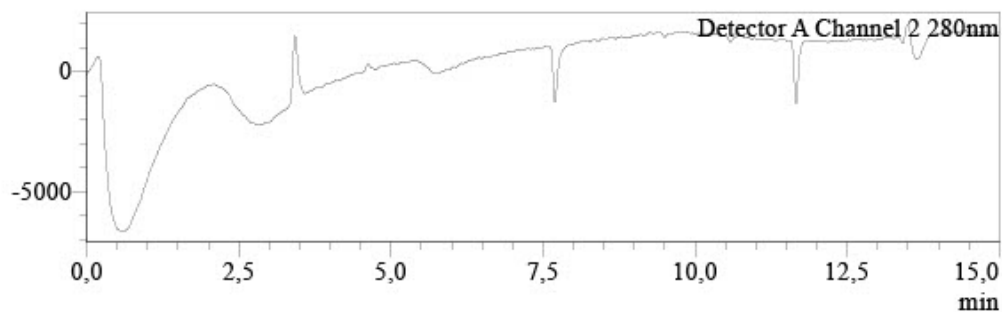

Peak Table

Detector A Channel 1 260nm

Peak#	Name	Ret. Time	Conc.	Unit	Area%
1	Benzyl Alcohol	3.418	1.026	% (m/m)	100.000
Total					100.000

Peak Table

Detector A Channel 2 280nm

Peak#	Name	Ret. Time	Conc.	Unit
Total				

Endotoxin Determination Report




File Information

Filename: C:\UVVis-Data\Data\File_260723_122453.vqud
Date/Time: 07/23/2026 01:13:01 PM

Instrument Information

Instrument Type: UV-1900 Series
Model (S/N): UV-1900i (A12536253123)

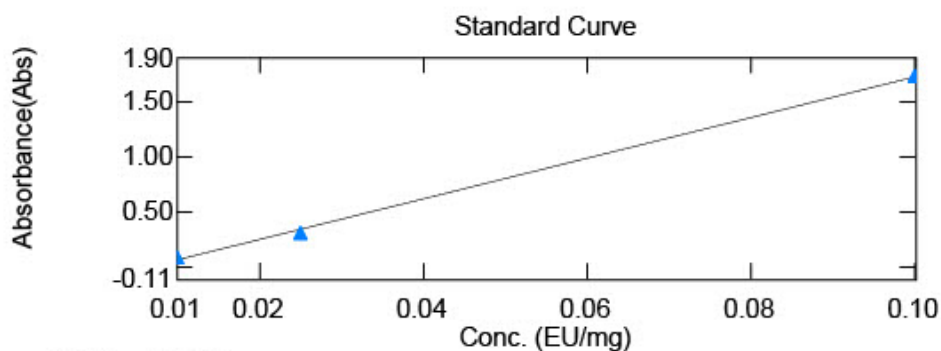

$$y = 18.5422x - 0.127539$$
$$r^2 = 0.99855$$

	Sample Name	Conc	Raw_WL545.0	Dilution Rate
1	LYO-0389	0.756	0.5732	20.00
2	LYO-0390	0.211	0.0677	20.00
3	LYO-0391	0.802	0.6164	20.00
4	LYO-0392	0.275	0.1271	20.00
5	LYO-0393	0.231	0.0863	20.00
6	LYO-0394	0.171	0.0309	20.00
7	LYO-0395	0.285	0.1364	20.00
8	LYO-0396	0.199	0.0569	20.00
9	LYO-0397	0.209	0.0660	20.00
10	LYO-0398	0.159	0.0201	20.00
11	LYO-0399	0.174	0.0337	20.00
12	LYO-0400	0.360	0.2067	20.00
13	LYO-0401	0.203	0.0605	20.00
14	LYO-0404	0.204	0.0613	20.00
15	LYO-0405	1.231	1.0135	20.00
16	LYO-0406	0.160	0.0206	20.00
17	LIQ-0039	0.008	0.0270	1.00

Responsibles



Mr. Ján Galbavý
CEO

Analysis results relate only to the samples tested.

This document shall not be reproduced except in full, without the written approval of Liquilabs s.r.o.